

## iSpindel Calibration

Gravity Unit: Specific Gravity(eg. 1.050) ▾

---


Measurement: Refractometer ▾

Reading: 1.006 ☐ Temperature Corrected. Wort Temperature 20 CAL@ 20 Celsius(°C) ▾

---

Tilt: 30.49 SG: 1.006 Add Data

	Tilt	SG	Degree 1 Value	Degree 1 Error	Degree 2 Value	Degree 2 Error	Degree 3 Value	Degree 3 Error
X	26.1	1.0000	0.9990	-0.0010	1.0003	0.0003	0.9993	-0.0007
X	30.49	1.0060	1.0067	0.0007	1.0069	0.0009	1.0073	0.0013
X	33.84	1.0130	1.0125	-0.0005	1.0121	-0.0009	1.0130	0.0000
X	42.8	1.0290	1.0281	-0.0009	1.0268	-0.0022	1.0273	-0.0017
X	52.5	1.0410	1.0450	0.0040	1.0440	0.0030	1.0433	0.0023
X	57.59	1.0540	1.0538	-0.0002	1.0535	-0.0005	1.0526	-0.0014
X	65.66	1.0700	1.0679	-0.0021	1.0694	-0.0006	1.0701	0.0001

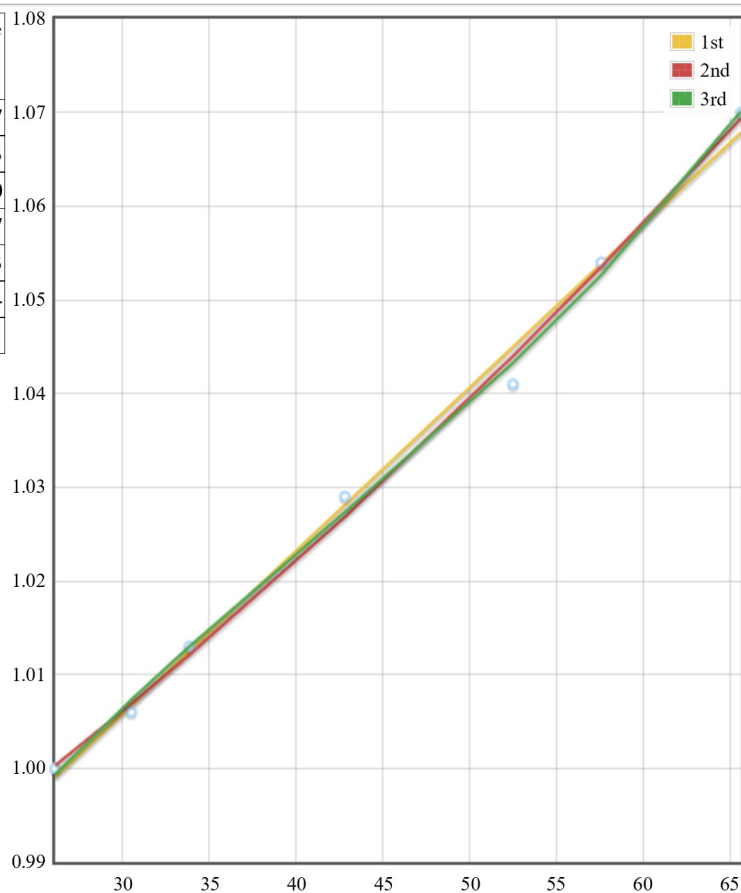

Degree 1:  $0.9536110970169976 + 0.0017403143274031245 \cdot \text{tilt}$

Degree 2:  $0.9665992629996584 + 0.0011100195230369539 \cdot \text{tilt} + 0.000006935066550235991 \cdot \text{tilt}^2$

Degree 3:  $0.9263814833764583 + 0.004006631096810417 \cdot \text{tilt} - 0.00005879929466053554 \cdot \text{tilt}^2 + 4.740034092995637e-7 \cdot \text{tilt}^3$